




SolidWorks Educational License
Instructional Use Only

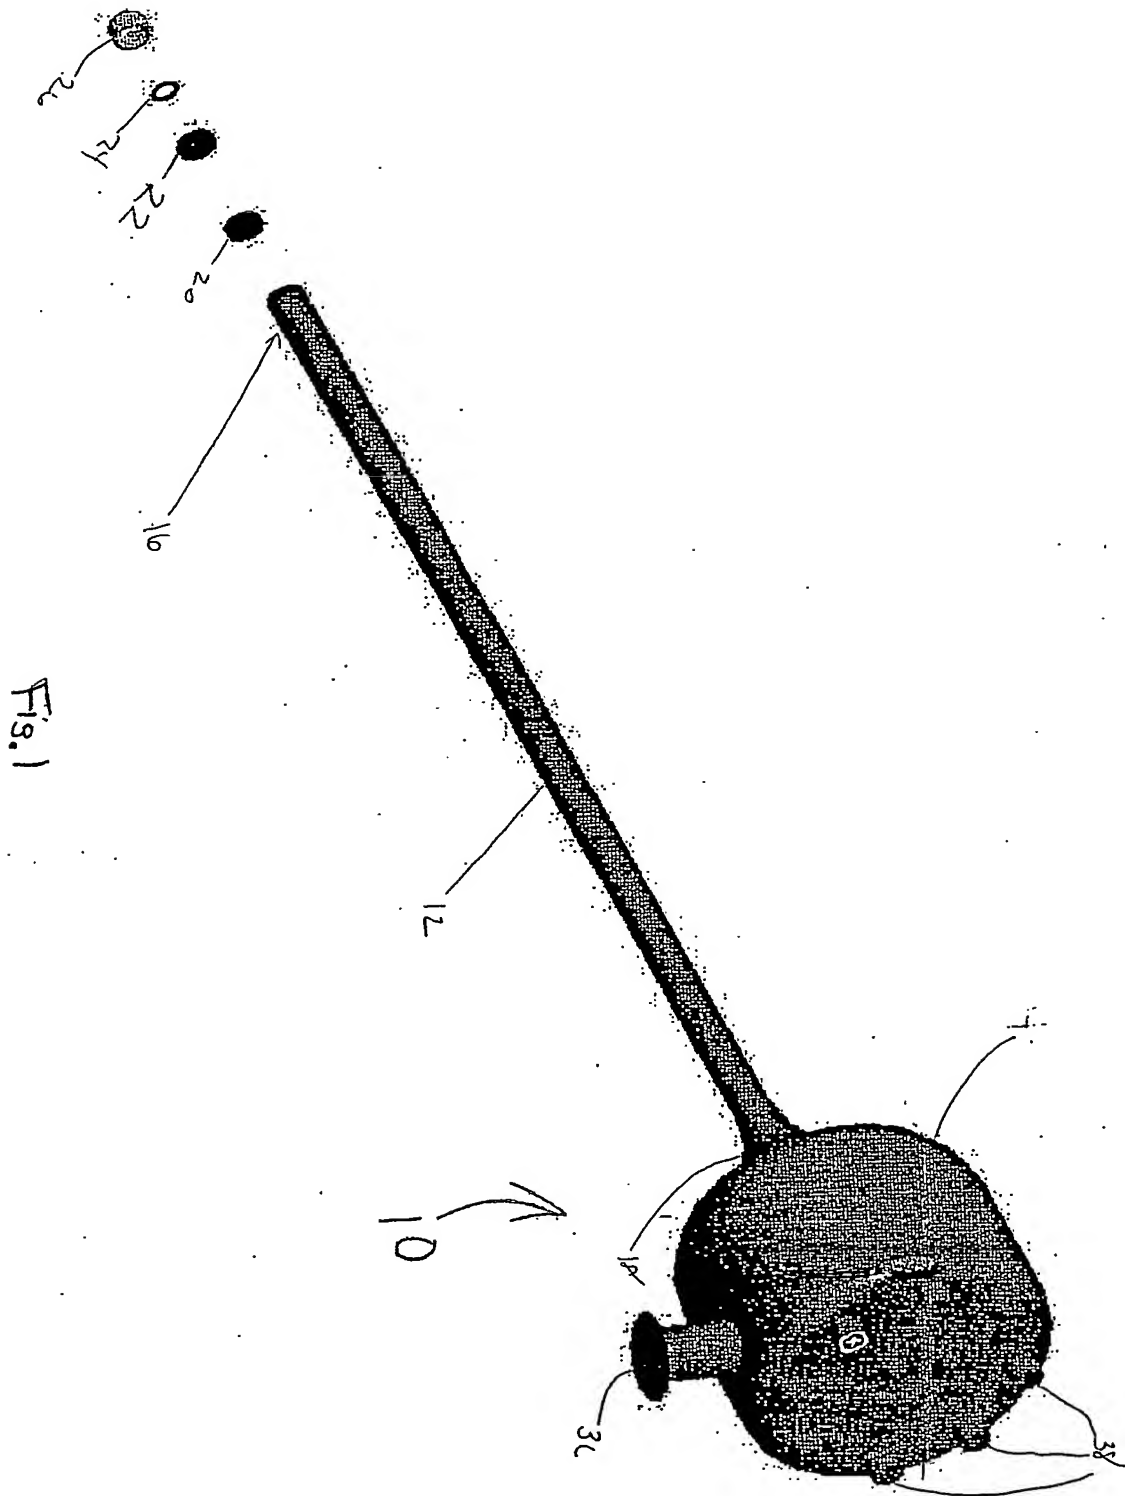

BEST AVAILABLE COPY

THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF CHILDRENS HOSPITAL BOSTON. ANY REPRODUCTION IN PART OR WHOLE WITHOUT THE WRITTEN PERMISSION OF CHILDRENS HOSPITAL BOSTON IS PROHIBITED.



Urethane Disk

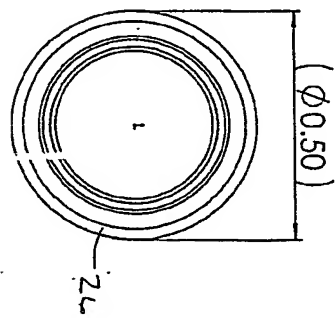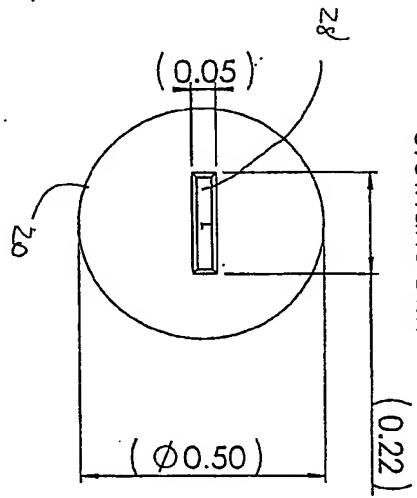

Rubber Gasket



FIG 2.

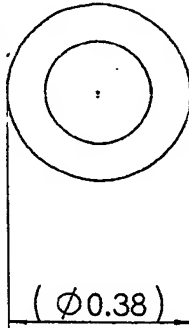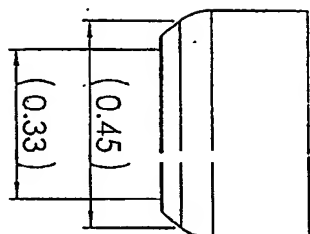

SolidWorks Educational License
Instructional Use Only

ITEM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION		MATERIAL SPECIFICATION	QTY REQD
PARTS LIST					
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN CM TOLERANCES ARE:		CAD GENERATED DRAWING, DO NOT MANUALLY UPDATE		CHILDRENS HOSPITAL-BOSTON	
FRACTIONS DECIMALS ANGLES		APPROVALS	DATE	MSD 770024 178719	
+/- .001		DRAWN JWC, MD	6/22/2002		
MATERIAL		CHECKED	RESP ENG		
FINISH		INT'G ENG			
NEXT ASSY		USED ON			
APPLICATION		DO NOT SCALE DRAWING	QUAL ENG		
SIZE		DWG. NO.		REV.	
A					

BEST AVAILABLE COPY

THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF CHILDREN'S HOSPITAL BOSTON. ANY REPRODUCTION IN PART OR WHOLE WITHOUT THE WRITTEN PERMISSION OF CHILDREN'S HOSPITAL BOSTON IS PROHIBITED.

SolidWorks Educational License
Instructional Use Only

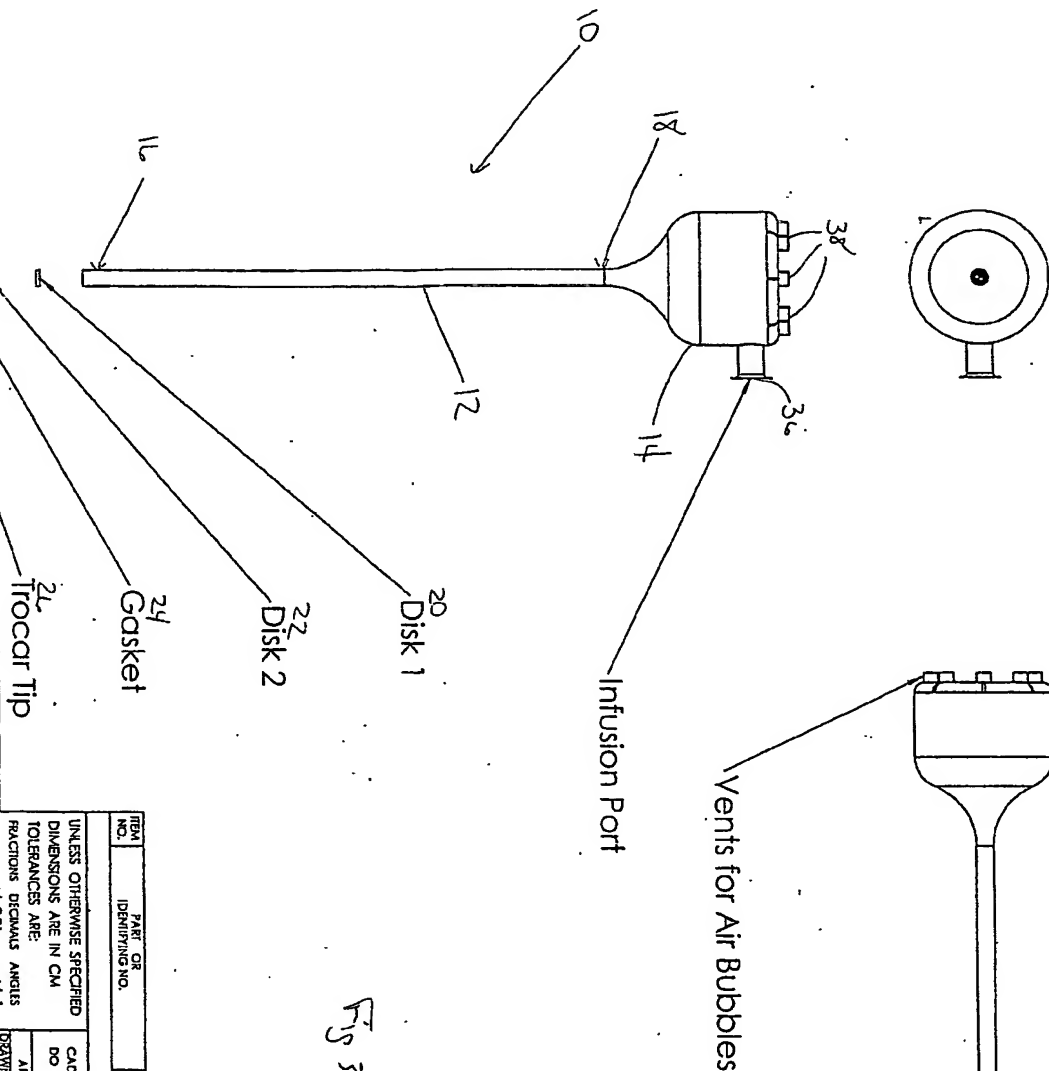


Fig 3

ITEM NO.		PART OR IDENTIFYING NO.		NOMENCLATURE OR DESCRIPTION		MATERIAL SPECIFICATION		QTY REQD	
<p>UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN CM TOLERANCES ARE: FRACTIONS DECIMALS ANGLES +/- .001 +/- .1</p>									
PARTS LIST				<p>CAO GENERATED DRAWING, DO NOT MANUALLY UPDATE</p> <p>APPROVALS: DRAWN: JWC, MD DATE: 6/12/2002</p> <p>CHECKED: RES' ENG: PRO ENG: QUAL ENG:</p>					
MATERIAL: --				<p>CHIL DREN'S HOSPITAL - BOSTON</p> <p>Trocort Assembly</p>					
FINISH: --				<p>SITE: DRWG NO. 1</p> <p>SCALE: 1:1</p> <p>CAO FILE: 1</p>					
DO NOT SCALE DRAWING				<p>APPROVALS: NEXT ASSY: USED ON: APPLICATION:</p>					

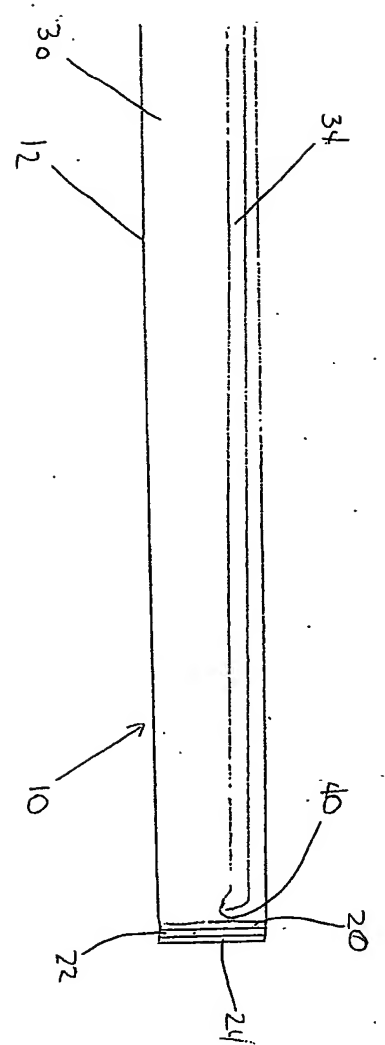


Fig. 4

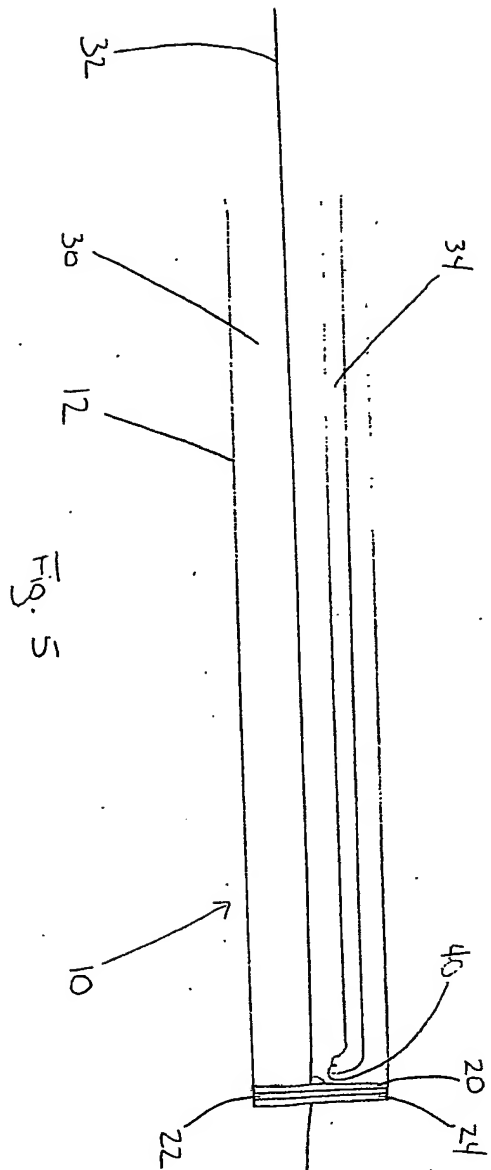


Fig. 5